



FIG. 1

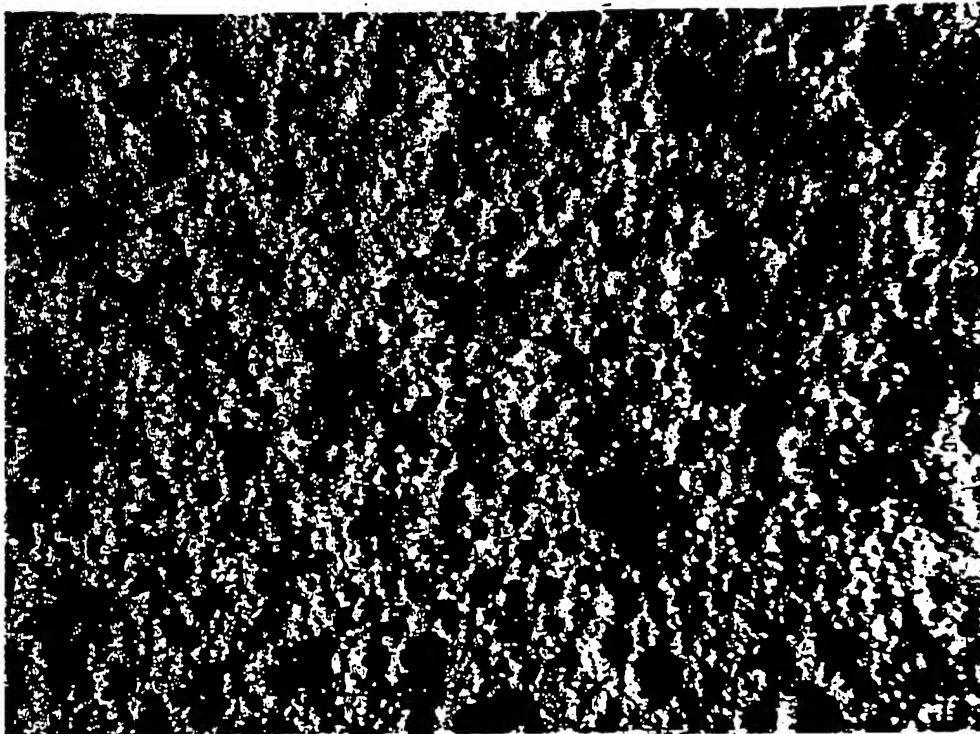

Injected Sample

1 millimeter

These two images were taken at the same magnification

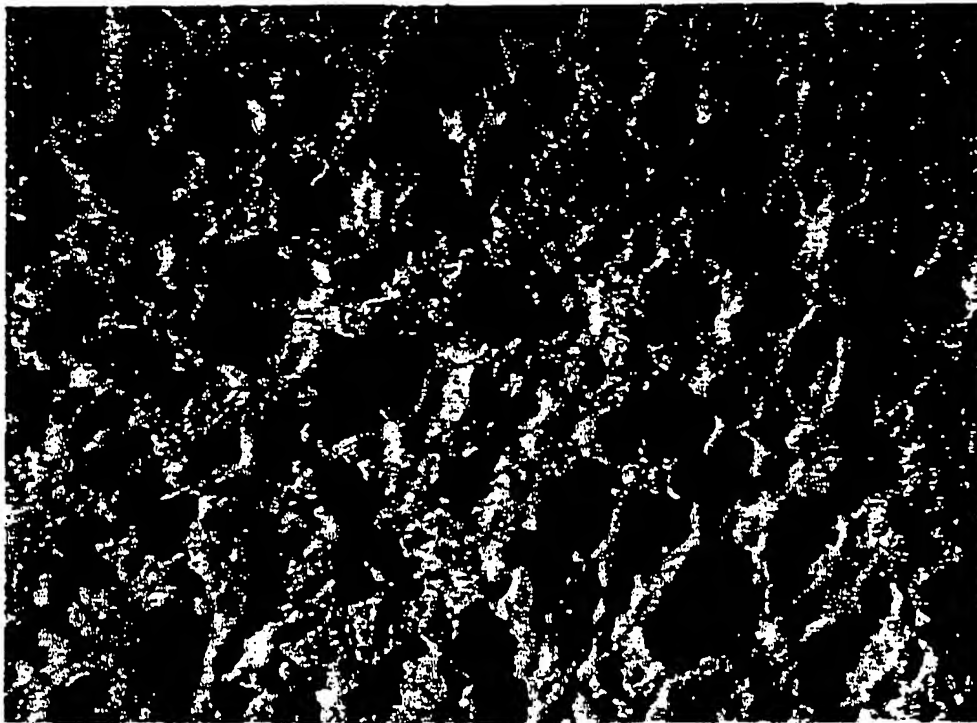


Uninjected Sample

1 millimeter

FIG. 2

U.S. GOVERNMENT PRINTING OFFICE: 1964 O - 344-100

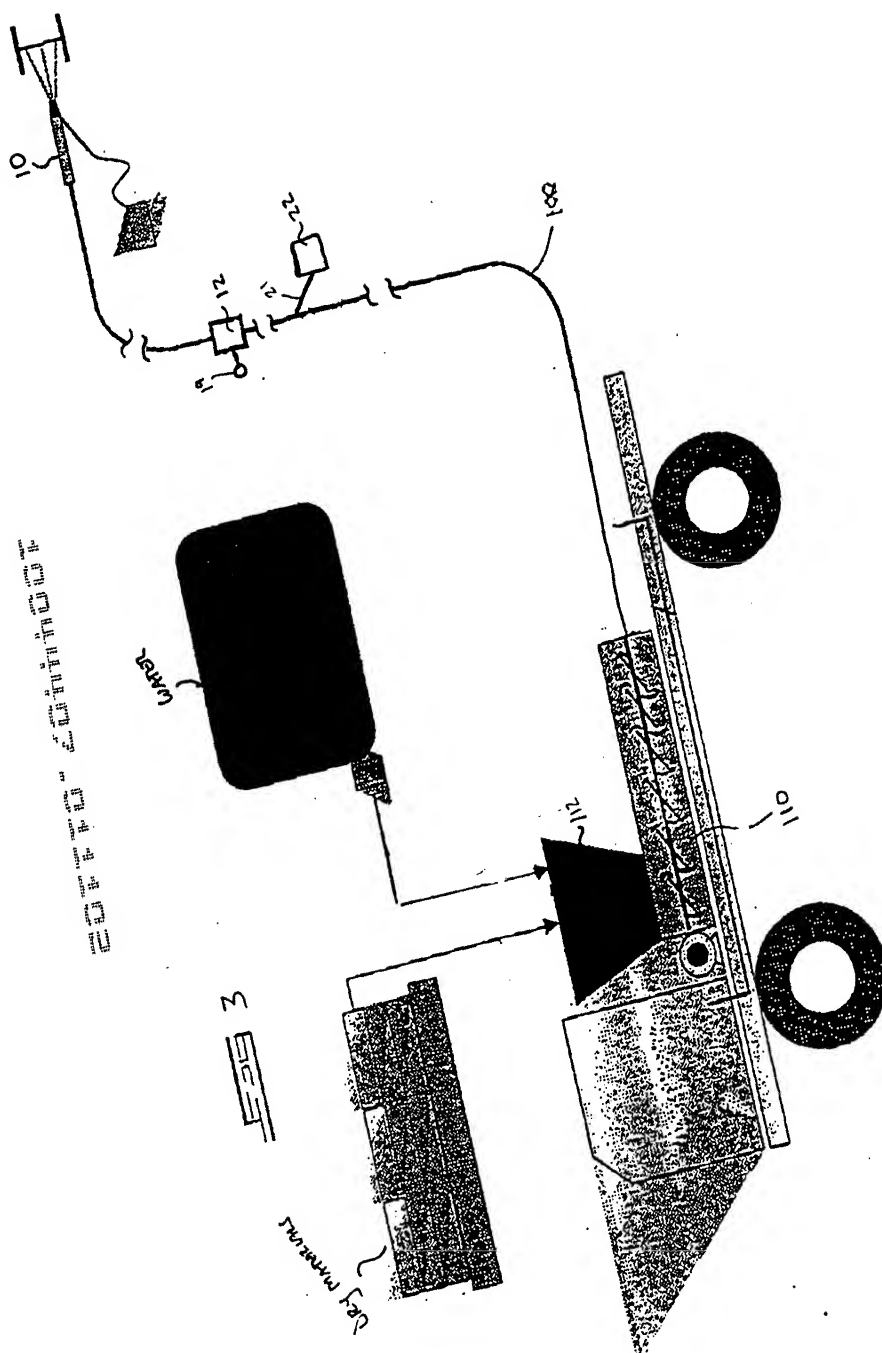

SEE FIG. 2

3

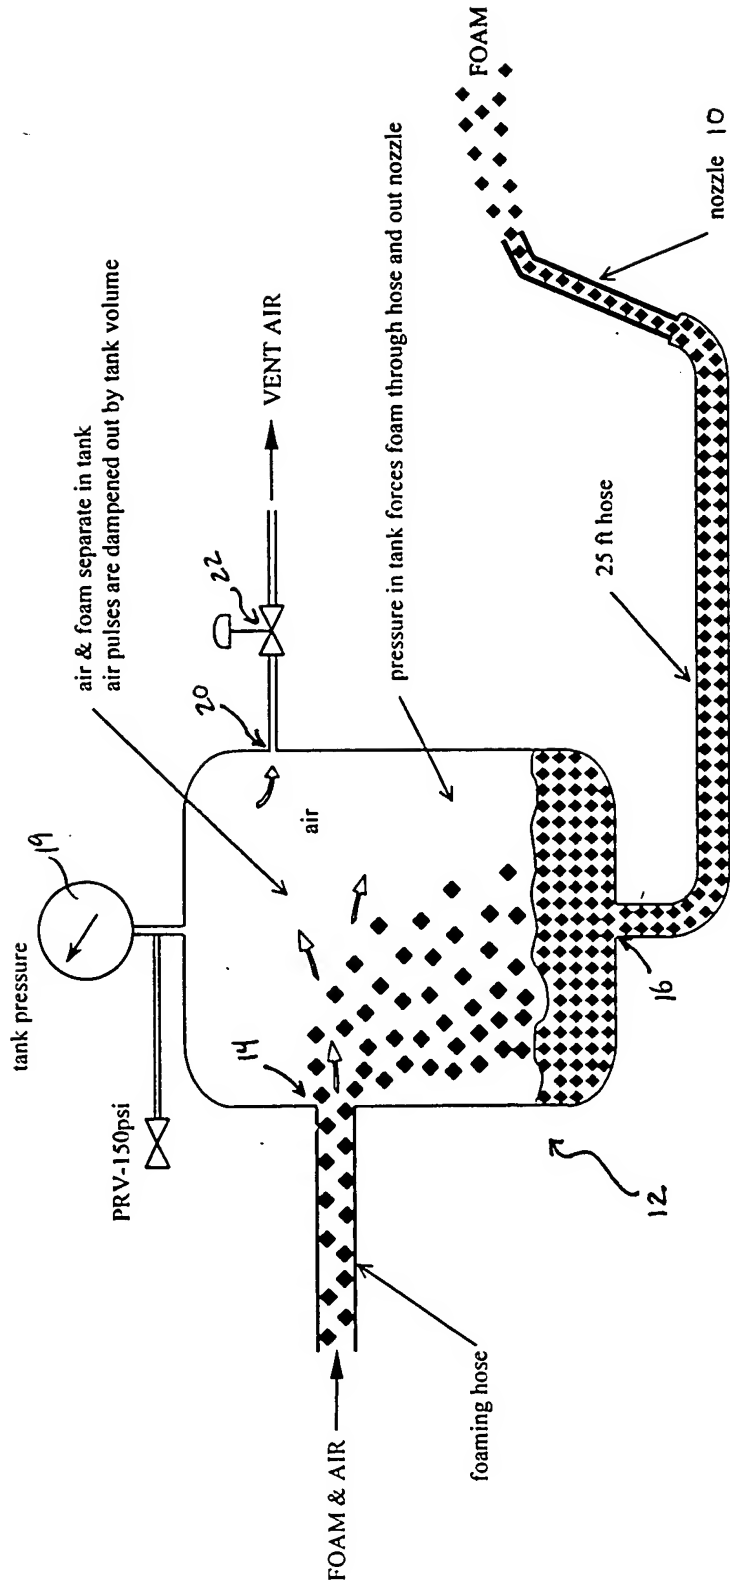


FIG. 4